


FPD310-FV Operating Manual


Freespace High Sensitivity PIN Photo Detector Unit
(400-1000nm)

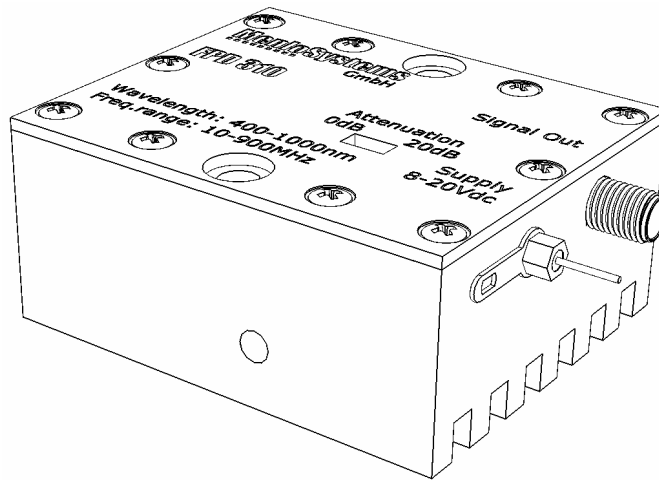

Product Specifications

Optical Input	Freespace
Supply Voltage	+9 to +20 V
Current Consumption	250 mA
Max. Incident Power	2 mW
Operating Temperature	10-40 °C
Spectral Range	400-1000 nm
Detector Diameter	0.4 mm
Frequency Range	1-1500 MHz
3dB-Bandwidth	10-900 MHz

Rise Time	0.7 ns
Gain - Setting 1	5×10^4 V/W
- Setting 2	5×10^2 V/W
Dark State Noise Level	-90 dBm
NEP (calculated)	$30 \text{ pW/Hz}^{1/2}$
Output Connector	SMA
Output Impedance	50Ω
Device Dimensions (mm)	60x50x27
Output Coupling	AC

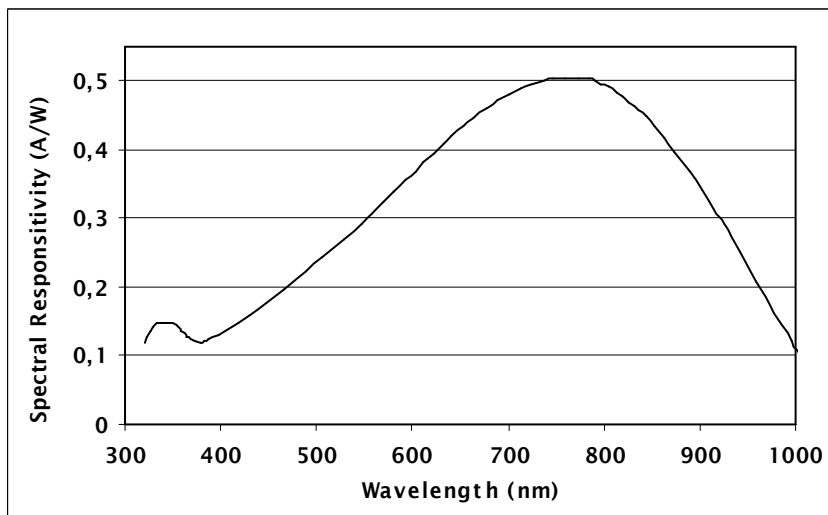


Packing Information

When unpacking your FPD310-FV, please check that the case contains the following items:

- 1x FPD310-FV Detector (with markings “FPD310” / “400-1000nm”)
- 1x Envelope with manual and test report

Setup and Operation

- After unpacking, connect the power supply to the detector as depicted in the following sketch; refer to technical drawings and labelling of the device to locate the respective connectors:



Best performance of the detector can be achieved when using a linear regulated power supply. Note that switched power supplies may introduce switching noise that could potentially carry through to the output signal.

- Connect **Signal Out** (SMA jack) to a suitable monitoring device, e.g. oscilloscope or RF-spectrum-analyzer, with 50Ω impedance.
Mount the device firmly in your setup using the mounting holes (at least one of the two holes through the device or M4-threaded hole at the side). Please note that when the device is not mounted properly, involuntary displacements during operation might occur, leading to uncontrolled reflections from the device.
- Switch on the power supply and monitoring device, and apply a light source to the photo diode.
- The FPD310-FV can be attenuated by 20dB operating the switch beneath the top with a small pen.

Maintaining the FPD310-FV

There are no serviceable parts in the FPD310-FV. The housing may be cleaned by wiping with a soft damp cloth. Do not use any alcohol or organic solvent to clean the mechanical parts. The window of the photo diode should only be cleaned using isopropyl alcohol and optical grade wipes.

If you suspect a problem with your FPD310-FV please contact Menlo Systems and technical support will be happy to assist you. For service requests, please make sure to provide the serial number of your device. For storage and shipping, please use the case your detector was shipped with.